



Simec AG

Areal Bleiche West Postfach 413 CH - 4800 Zofingen
Telefon +41 62 752 83 08 Fax +41 62 752 83 09
E-Mail: info@simec.ch www.simec.ch

Test report

Number **C 42571**

Object of analysis: Trenbolone Hexahydrobenzylcarbonate

Customer: Frank Dawson

Samples: 1

Batch: -

Receipt: 30.03.2016

Subject: Trenbolone Hexahydrobenzylcarbonate: Assay, Identification

Method(s): HPLC

Sample / Analysis:	Method	Status	Result	Specification	complies
<u>Trenbolone Hexahydrobenzylcarbonate:</u>					
Identification	HPLC	N	complies	complies	yes
Content	HPLC	N	96.9 %	-	-

Method-status: G = GMP A = accredited V = generally validated P = validated on product N = not validated
E = external lab

Remarks: The sample(s) mentioned above have been analysed as they have been sent to us by the client. We have not controlled external processes like manufacturing, labelling, sampling, shipping, storage. These results are for information only and do not compensate for correct quality control by the manufacturer/distributor. Generally, pharmaceutical products have to be produced and distributed under full GMP/GDP regime, including GMP-compliant analyses with validated methods.

Signatures: controlled & released. 

Staff: 

completed:

27.05.2016

The enclosed results refer exclusively to the object of examination described above. The measuring accuracy is available on request. Only handwritten signatures are valid. Without written permission, it is not allowed to publish single parts of this report.

page 1 of 1




S SCHWEIZERISCHER PRÜFSTELLENDIENST
T SERVICE SUISSE D'ESSAI
S SERVIZIO DI PROVA SVIZZERA
S SWISS TESTING SERVICE

Zertifiziert Swissmedic GMP / PIC

STS 443 nach EN 17 025

Report steroid analysis

HPLC:	Nr.5	Druckdatum:	17.05.2016 08:35:36
Analysendatum:	15.05.2016 00:19:14	Injektvolumen:	20
Vial:	169		
Probenidentifikation:	C42571 A		
Operator:	admin		
Chrom.-Beding.	ACN / Wasser, gradient		
Temperatur:	40 °C		
Säule	Nr. 121, 250 x 4,6, C18		
Detektion:	UV 240nm		

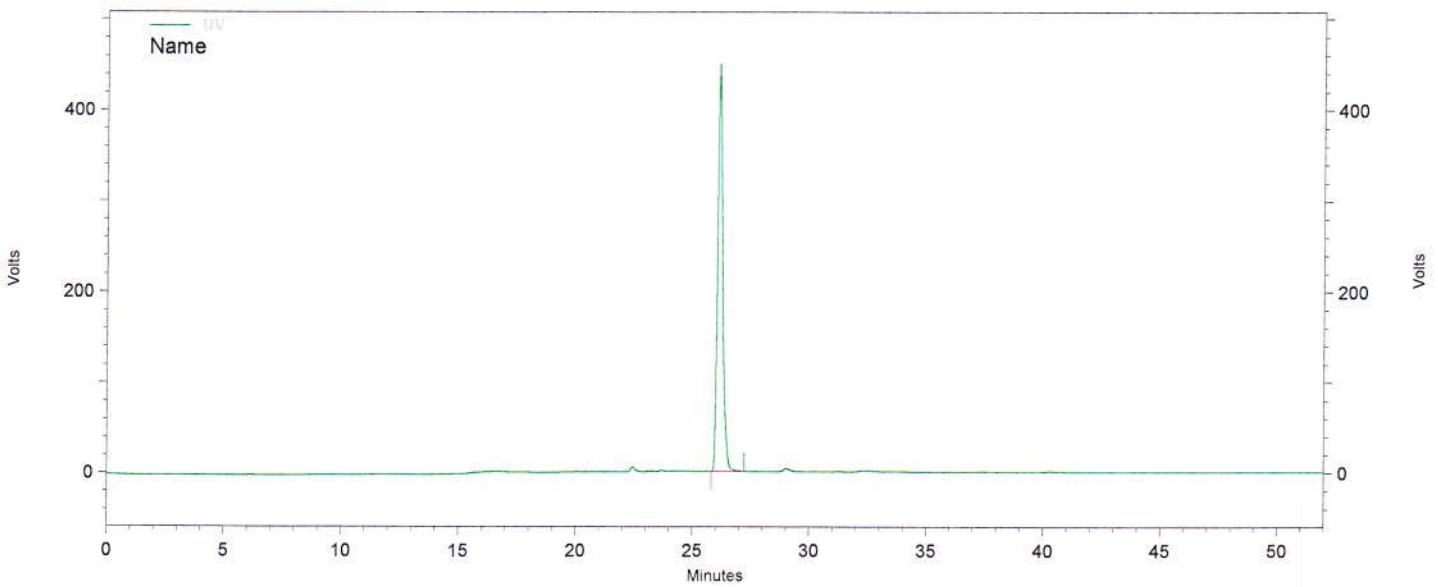

Channel A


UV Results

Name	Time	Area	Amount	Area Percent
Trenbolone acetate			0,000 BDL	
Nandrolone Phenylpropionate			0,000 BDL	
	26,120	27164453	0,000	100,000
Trenbolone			0,000 BDL	
Hexahydrobenzylcarbonat				
Testosterone enanthate			0,000 BDL	
Testosterone cypionate			0,000 BDL	
Totals		27164453	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2016\Mai 2016\02,05,16\Diverse Steroide\127_C42571 A-Rep1.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC:	Nr.5	Druckdatum:	17.05.2016 08:35:41
Analysendatum:	15.05.2016 01:12:39	Injektvolumen:	20
Vial:	169		
Probenidentifikation:	C42571 A		
Operator:	admin		
Chrom.-Beding.	ACN / Wasser, gradient		
Temperatur:	40 °C		
Säule	Nr. 121, 250 x 4,6, C18		
Detektion:	UV 240nm		

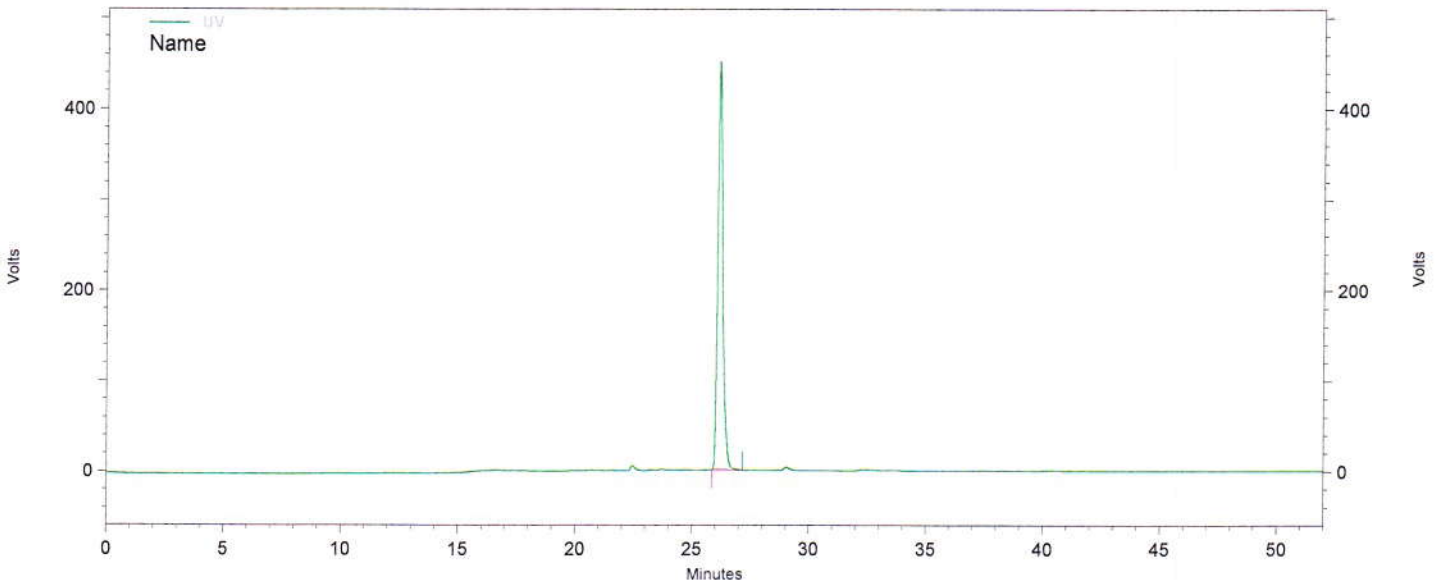

Channel A


UV Results

Name	Time	Area	Amount	Area Percent
Trenbolone acetate			0,000 BDL	
Nandrolone Phenylpropionate			0,000 BDL	
	26,137	27081701	0,000	100,000
Trenbolone			0,000 BDL	
Hexahydrobenzylcarbonat				
Testosterone enanthate			0,000 BDL	
Testosterone cypionate			0,000 BDL	
Totals		27081701	0,000	100,000

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2016\Mai 2016\02,05,16\Diverse Steroide\127_C42571 A-Rep2.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC:	Nr.5	Druckdatum:	17.05.2016 08:35:45
Analysendatum:	15.05.2016 02:05:57	Injektvolumen:	20
Vial:	169		
Probenidentifikation:	C42571 A		
Operator:	admin		
Chrom.-Beding.	ACN / Wasser, gradient		
Temperatur:	40 °C		
Säule	Nr. 121, 250 x 4,6, C18		
Detektion:	UV 240nm		

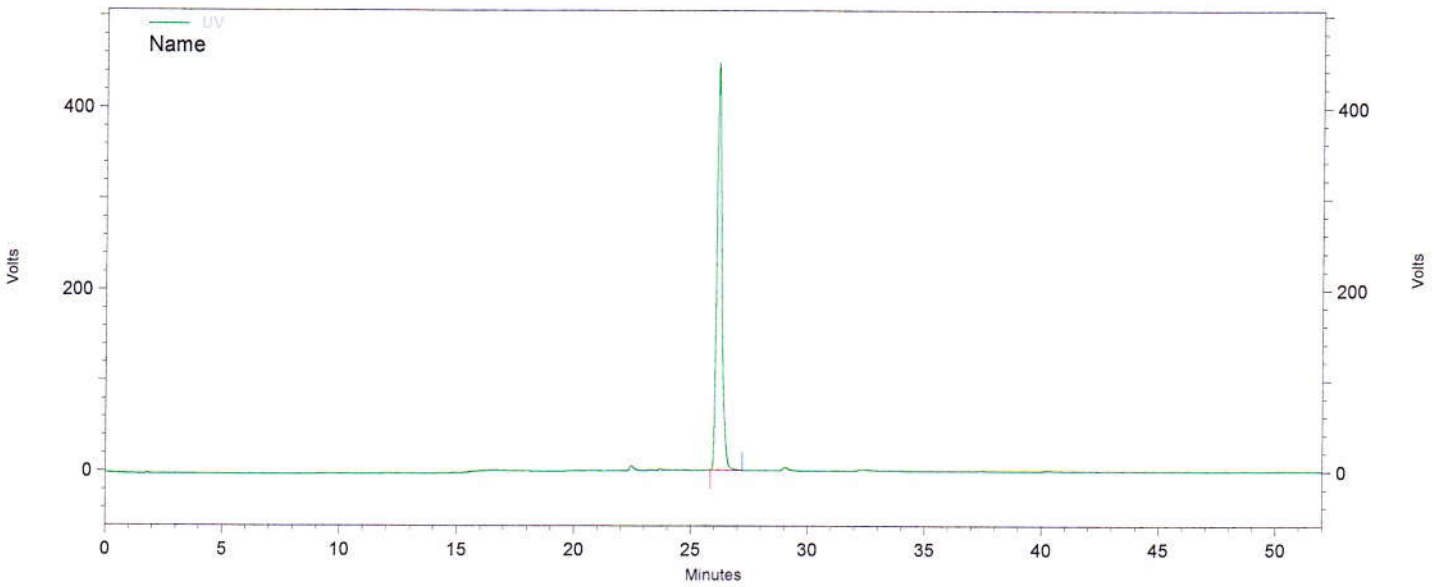

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Trenbolone acetate			0,000 BDL	
Nandrolone Phenylpropionate			0,000 BDL	
	26,133	26997759	0,000	100,000
Trenbolone			0,000 BDL	
Hexahydrobenzylcarbonat				
Testosterone enanthate			0,000 BDL	
Testosterone cypionate			0,000 BDL	

Totals		26997759	0,000	100,000
--------	--	----------	-------	---------

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2016\Mai 2016\02,05,16\Diverse Steroide\127_C42571 A-Rep3.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC:	Nr.5	Druckdatum:	17.05.2016 08:35:49
Analysendatum:	15.05.2016 02:59:17	Injektvolumen:	20
Vial:	170		
Probenidentifikation:	C42571 B		
Operator:	admin		
Chrom.-Beding.	ACN / Wasser, gradient		
Temperatur:	40 °C		
Säule	Nr. 121, 250 x 4,6, C18		
Detektion:	UV 240nm		

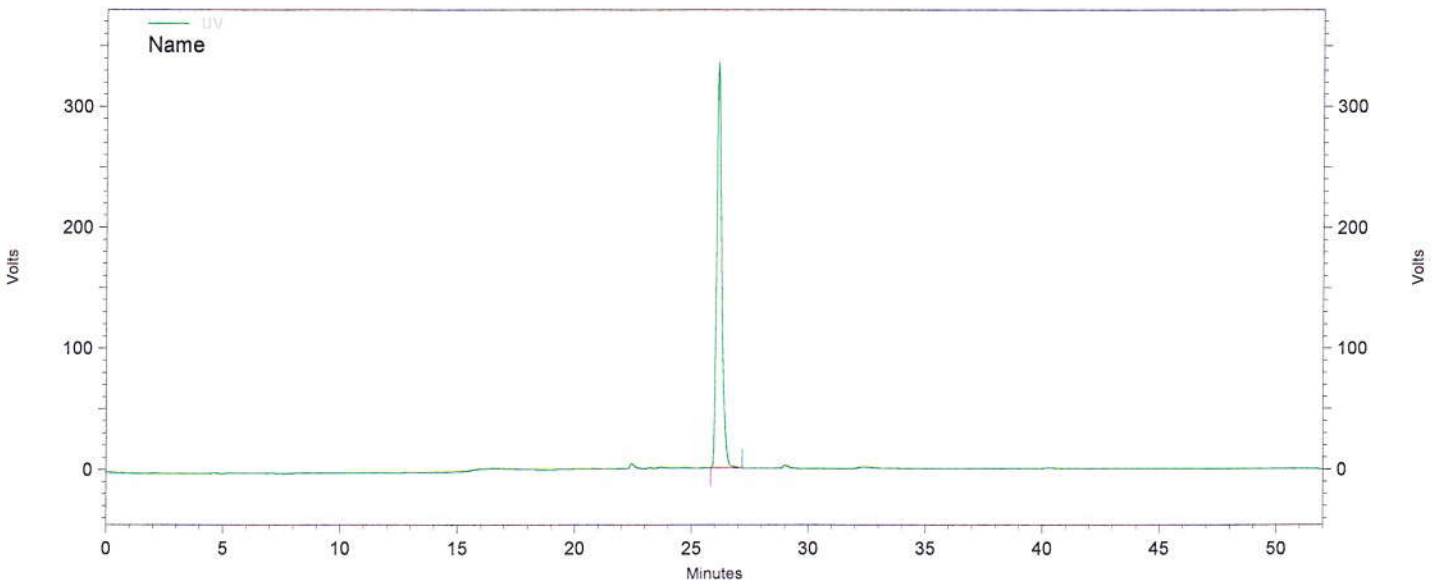

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Trenbolone acetate			0,000 BDL	
Nandrolone Phenylpropionate	26,120	20274477	0,000	100,000
Trenbolone			0,000 BDL	
Hexahydrobenzylcarbonat				
Testosterone enanthate			0,000 BDL	
Testosterone cypionate			0,000 BDL	

Totals		20274477	0,000	100,000
--------	--	----------	-------	---------

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2016\Mai 2016\02,05,16\Diverse Steroide\128_C42571 B-Rep1.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC:	Nr.5	Druckdatum:	17.05.2016 08:35:53
Analysendatum:	15.05.2016 03:52:39	Injektvolumen:	20
Vial:	170		
Probenidentifikation:	C42571 B		
Operator:	admin		
Chrom.-Beding.	ACN / Wasser, gradient		
Temperatur:	40 °C		
Säule	Nr. 121, 250 x 4,6, C18		
Detektion:	UV 240nm		

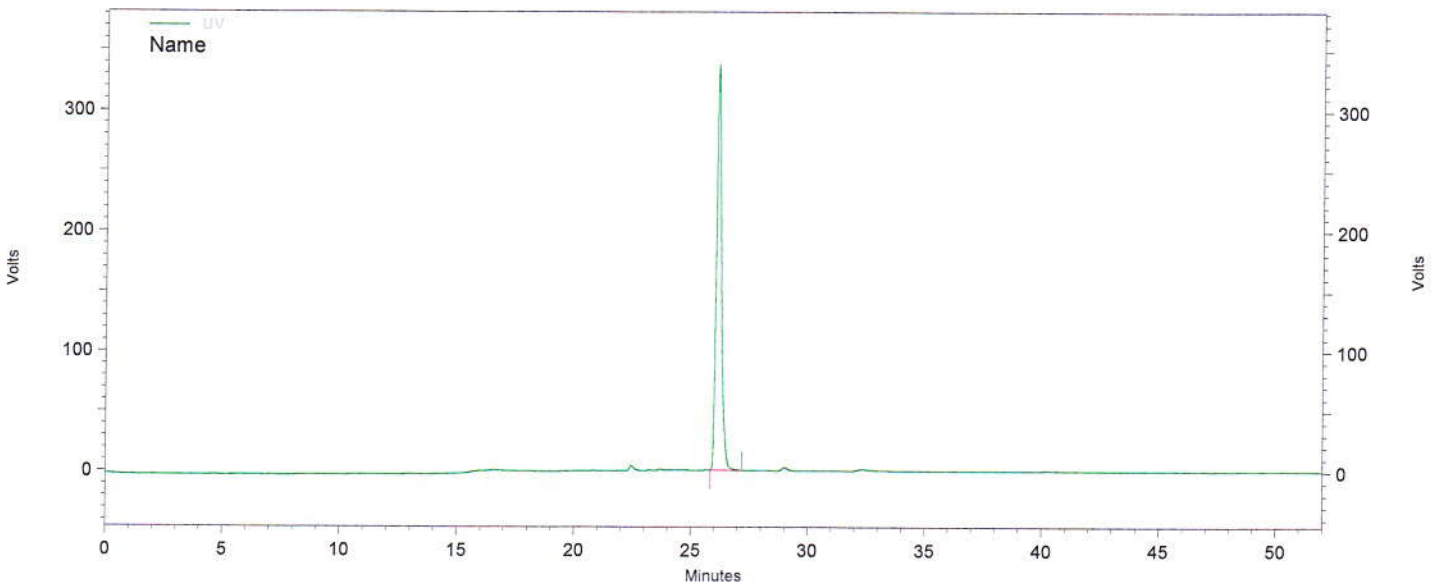

Channel A

UV Results


Name	Time	Area	Amount	Area Percent
Trenbolone acetate			0,000 BDL	
Nandrolone Phenylpropionate			0,000 BDL	
	26,110	20338321	0,000	100,000
Trenbolone			0,000 BDL	
Hexahydrobenzylcarbonat				
Testosterone enanthate			0,000 BDL	
Testosterone cypionate			0,000 BDL	

Totals		20338321	0,000	100,000
--------	--	----------	-------	---------

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2016\Mai 2016\02,05,16\Diverse Steroide\128_C42571 B-Rep2.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met

Report steroid analysis

HPLC:	Nr.5	Druckdatum:	17.05.2016 08:35:58
Analysendatum:	15.05.2016 04:45:56	Injektvolumen:	20
Vial:	170		
Probenidentifikation:	C42571 B		
Operator:	admin		
Chrom.-Beding.	ACN / Wasser, gradient		
Temperatur:	40 °C		
Säule	Nr. 121, 250 x 4,6, C18		
Detektion:	UV 240nm		

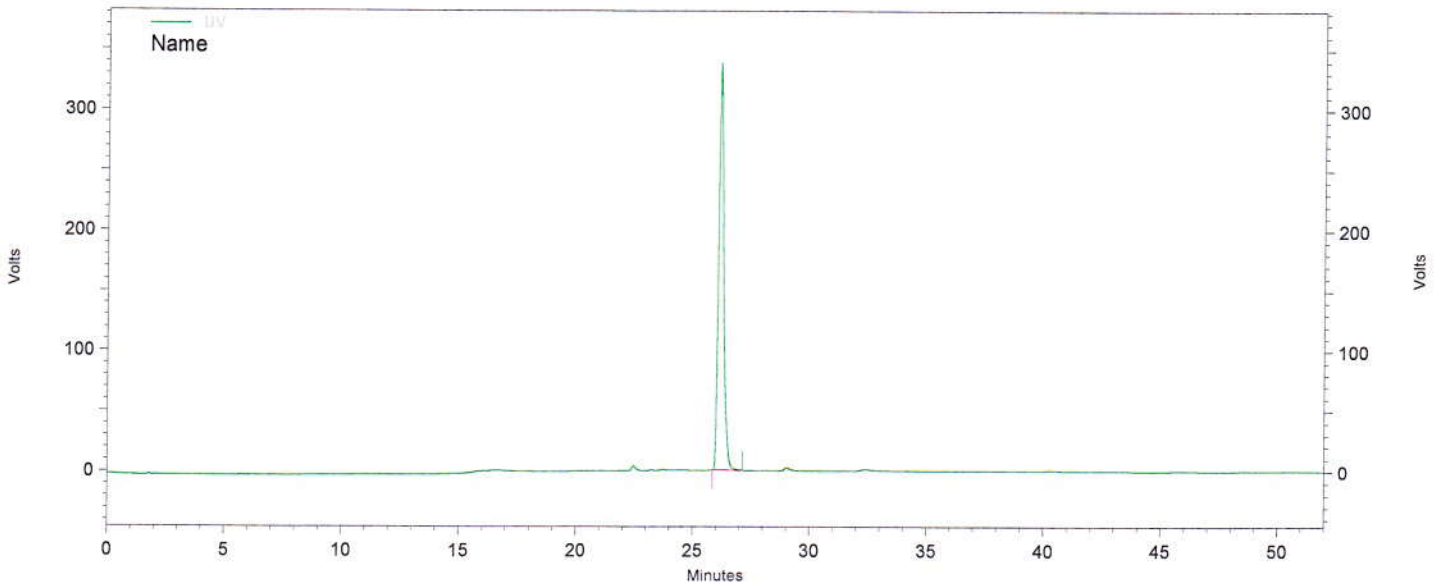

Channel A

UV Results

Name	Time	Area	Amount	Area Percent
Trenbolone acetate			0,000 BDL	
Nandrolone Phenylpropionate			0,000 BDL	
	26,137	20311431	0,000	100,000
Trenbolone			0,000 BDL	
Hexahydrobenzylcarbonat				
Testosterone enanthate			0,000 BDL	
Testosterone cypionate			0,000 BDL	

Totals		20311431	0,000	100,000
--------	--	----------	-------	---------

Daten File: C:\EZChrom Elite\Enterprise\Projects\Simec\Data\2016\Mai 2016\02,05,16\Diverse Steroide\128_C42571 B-Rep3.dat
 Methode: C:\EZChrom Elite\Enterprise\Projects\Simec\Method\Steroide\Steroide A.met